



**Please note that Cypress is an Infineon Technologies Company.**

The document following this cover page is marked as “Cypress” document as this is the company that originally developed the product. Please note that Infineon will continue to offer the product to new and existing customers as part of the Infineon product portfolio.

**Continuity of document content**

The fact that Infineon offers the following product as part of the Infineon product portfolio does not lead to any changes to this document. Future revisions will occur when appropriate, and any changes will be set out on the document history page.

**Continuity of ordering part numbers**

Infineon continues to support existing part numbers. Please continue to use the ordering part numbers listed in the datasheet for ordering.

## Infrared Thermometer using PSoC®

Author: Sanjeev Kumar K.

Associated Project: Yes

Associated Part Family: CY8C24x94, CY8C27xxx, CY8C28xxx, CY8C29xxx

Software Version: PSoC® Designer™ 5.4

Related Application Notes: For a complete list of the application notes, [click here](#).

To get the latest version of this application note, or the associated project file, please visit

<http://www.cypress.com/go/AN58829>

This application note describes how to build an infrared thermometer using PSoC® 1. This application note also discusses the theory of Infrared thermometers in brief. This design uses no external active components to buffer, amplify, and detect the signal source.

## Contents

Introduction .....	1
Infrared Thermometer Principle.....	1
Steps to Calculate Object Temperature .....	2
Measure Thermopile Voltage .....	2
Measure Thermistor Resistance (Ra) and Calculate Ambient Temperature.....	3
Object temperature calculation.....	3
Software .....	3
Create Lookup Table .....	5
Read ADC Values .....	5
Process ADC Values for Temperature .....	5
Schematic .....	7
Accuracy of Object Temperature.....	8
Field of View Angle.....	8
Casing and Optics in the Sensor .....	8
Distance between Sensor and Object .....	8
Calibration .....	9
Summary.....	10
Related Application Notes .....	10
Worldwide Sales and Design Support.....	12

## Introduction

Infrared thermometers are widely used in medical and industrial applications.

- They measure temperature without any contact with the object for measurement.
- They measure a wide range of temperature.
- Their accuracy is comparable with other types of thermometers.

## Infrared Thermometer Principle

Infrared thermometer uses thermopile sensor to measure temperature. Thermopile sensor has an IR absorber connected with a series of thermocouples. The cold contacts of the thermocouples are connected to a known reference. These thermocouples measure the object temperature. The ambient temperature of the sensor is measured using a thermistor.

Figure 1. Thermopile


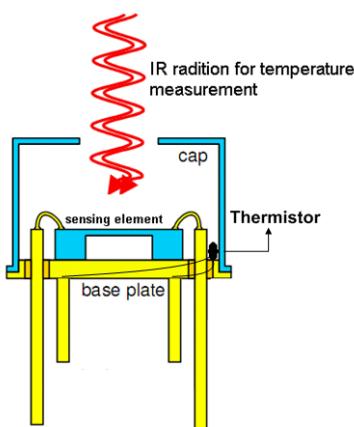


Figure 2. Thermopile Pin Details

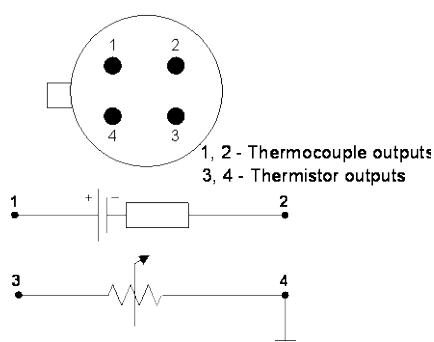

A thermopile sensor has four pins, two of them give the voltage across the series of thermocouples and the other two pins are used to measure thermistor resistance. The thermopile sensor generates a voltage, which is proportional to the incident infrared (IR) radiation power. You can deduct the object's temperature from the thermopile signal because every object emits IR radiation with a power, which is a strict function of its temperature.

The total radiation power  $P_{obj}$  emitted by an object of temperature  $T_{obj}$  can be expressed as Equation 1

$$\text{Equation 1} \quad P_{obj} = \sigma \cdot \varepsilon \cdot T_{obj}$$

with  $\sigma$  being the Stefan-Boltzmann constant and  $\varepsilon$  the so-called emission factor (or emissivity) of the object. In an ideal case  $\varepsilon$  has the values '1' and '0'. For most substances, the emission factor lies in the range 0.85 to 0.95. Equation 1 is called the Stefan-Boltzmann law.

The heat-balance equation relates the net power  $P_{rad}$  received by the thermopile to two temperatures:  $T_{obj}$  and  $T_{amb}$ . In most cases the instrument's temperature  $T_{obj}$  equals (or is near to) the temperature of the ambient  $T_{amb}$ . Therefore, refer to this value as  $T_a$ , the ambient

temperature. The total heat power  $P_{rad}$  received from the object at temperature  $T_{obj}$  is given to

$$\text{Equation 2} \quad P_{rad} = k \cdot \varepsilon \cdot (T_{obj}^4 - T_a^4)$$

Thermopile generates a voltage  $V_{tp}$  which is proportional to the incident radiation.


$$\text{Equation 3} \quad V_{tp} = S \cdot k \cdot \varepsilon \cdot (T_{obj}^4 - T_a^4)$$

$$\text{Equation 4} \quad V_{tp} = K(T_{obj}^4 - T_a^4)$$

Where  $S$  is sensitivity is calibration constant and  $\varepsilon$  is emissivity.

Usually, sensitivity of the thermocouple is in the range of microvolts if the ambient temperature is fixed. An empirical relation between  $V_{tp}$  and  $T_{obj}$  or a look up table gives the object temperature. From Equation 2 it is evident that  $V_{tp}$  changes according to changes in ambient temperature. This ambient temperature needs to be compensated to get the correct object temperature.

Figure 3. Block Diagram

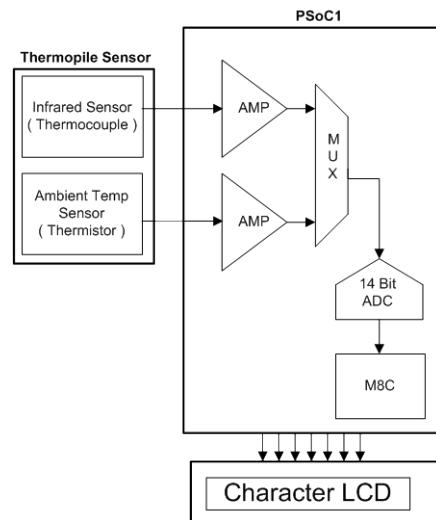

## Steps to Calculate Object Temperature

1. Measure thermopile voltage ( $V_{tp}$ )
2. Measure thermistor resistance ( $R_a$ ) and calculate ambient temperature ( $T_a$ )
3. Calculate ambient temperature compensation and object temperature

## Measure Thermopile Voltage

Usually the output of thermopile is in the order of a few  $\mu$ V, so take care for offset and SNR.

As an example, a sensor from Perkin Elmer TPS23B is used. The average sensitivity ( $\Delta V_{TP}/\Delta T$ ) of the thermopile is 50  $\mu$ V/K or 1.845 mV at 309.9K, which is the typical human body temperature.

Thermopile voltage can be amplified using correlated double sampling method (CDS). CDS is followed to reduce offset and low frequency noise cancellation. For more details on CDS, refer Application Note [AN2226, Correlated Double Sampling](#). A brief about this method is reproduced here for reference. Consider the two ends of a voltage source (thermopile) connected as the inputs to the programmable gain amplifier (PGA). This is then connected to the analog to digital convertor (ADC) that has offsets. The block diagram of the connections is shown in Figure 4.

When the MUX selection is input 1, the Vout would be as shown in Equation 3.

$$\text{Equation 5} \quad V_{out1} = V_{source} + V_{offset1} + V_{noise1}$$

When the MUX selection is changed to input 2, the Vout would be changed to Equation 4.

$$\text{Equation 6} \quad V_{out2} = V_{offset2} + V_{noise2}$$

$V_{offset1}$  and  $V_{offset2}$  are equal as the offset is constant over time. So when you subtract  $V_{out2}$  from  $V_{out1}$ , the offset is cancelled and the result is:


$$\text{Equation 7} \quad V_{tp} = V_{source} + V_{noise1} - V_{noise2}$$

The noise subtraction in time gives a result of low frequency noise cancelation response for the system .This response affects only the noise and not the actual signal, thus cancelling the low frequency noise. The details about the math for this waveform are given in [AN2226](#).

### IIR Filter

IIR low pass filter is implemented in software to reduce the high frequency noise. In other words, the implementation essentially takes a part of the old value and adds it to a part of the new value. The theory and implementation behind the IIR filter in software are provided in the Application Note [AN2099, Single-Pole IIR Filters](#). The voltage measurement for temperature sensor is well filtered by the CDS and IIR filter. The value is then used for both thermopile voltage and ambient temperature compensation.


Figure 4. Thermopile Connections Block Diagram

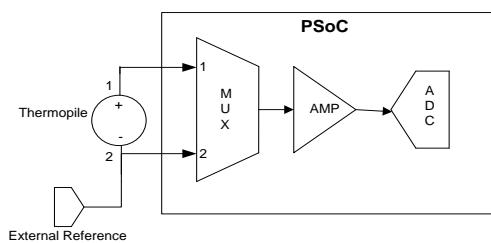

### Measure Thermistor Resistance ( $R_a$ ) and Calculate Ambient Temperature

Thermistor resistance can be measured by 'PSoC Style' as described in detail in the application note, [AN2017](#).

Figure 5. Thermistor Connection Block Diagram

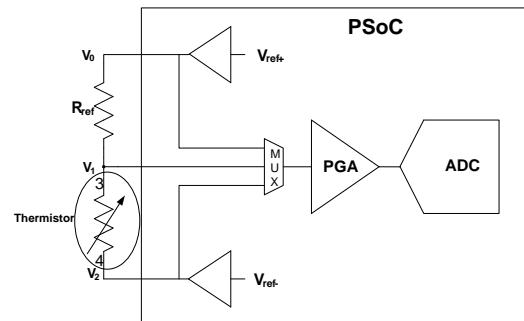

A voltage divider is constructed using a reference  $R_{ref}$  and thermistor inside the sensor.  $V_0$  and  $V_2$  are voltage references RefHi and RefLo from PSoC. A mux is switched between  $V_0$ ,  $V_1$ , and  $V_2$ . The signal from the mux is fed to a PGA of gain 'G', which is read by an ADC.

$$\text{Equation 8} \quad R_{thermistor} = R_{ref} * \left( \frac{V_1 - V_2}{V_0 - V_1} \right)$$

Find the thermistor value either in the thermistor lookup table provided by the sensor manufacturer or using Stein Harts equation to locate the ambient temperature  $T_a$ .

### Object temperature calculation

To calculate the object temperature, follow these steps:

1. Locate the equivalent temperature  $T_a$  in the lookup table provided by the sensor manufacturer.
2. Locate the equivalent temperature of  $V_{tp}$  (from Equation 5) to  $T_{tp}$ .
3. The object temperature is calculated by adding  $T_{tp}$  to  $T_a$ .


$$\text{Equation 9} \quad T_{obj} = T_{tp} + T_a$$

### Software

The software flow is as follows:

- Create lookup table
- Read ADC values for thermistor and thermo couple
- Process ADC values for temperature

Figure 6. Software Flow

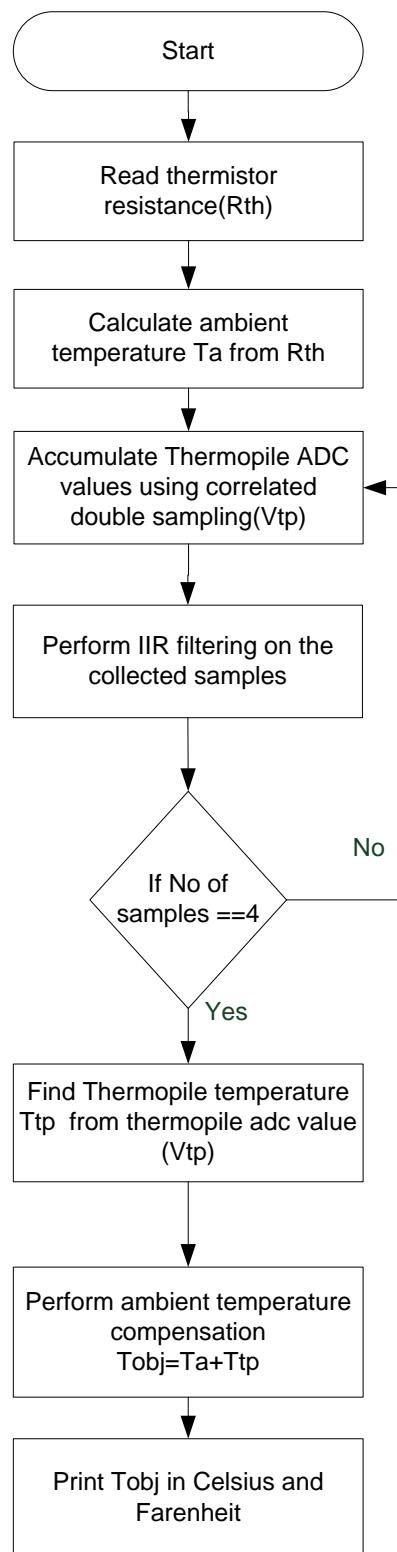

## Create Lookup Table

The lookup table for a thermistor is created using the table from Perkin-Elmer data sheet, which describes the thermistor's voltage against temperature characteristics.

Table 1. Thermistor Data

Temperature	Rnom	Temperature	Rnom
°C	Ω	°C	Ω
-20	915479	45	44175
-15	694575	50	36497
-10	531349	55	30303
-5	409715	60	25280
0	318336	65	21187
5	249149	70	17836
10	196369	75	15079
15	155815	80	12800
20	124439	85	10910
25	100000	90	9334
30	80843	95	8016
35	65732	100	6908
40	53743		

Table 1 has temperature mapped against resistance value. Consider Rnom ( $R_{th}$ ) as the nominal resistance. Thermistor can be calculated from [Equation 8](#).

Table 2. Thermocouple Data

Temperature	Typ	Temperature	Typ
°C	mV	°C	mV
-20	-1.55	40	0.71
-10	-1.29	50	1.25
0	-0.98	60	1.84
10	-0.61	70	2.48
20	-0.21	80	3.16
25	0	90	3.9
30	0.23	100	4.7

Table 2 represents the variation in thermopile voltage with temperature difference between the hot and cold ends of the thermopile. The reference temperature is taken as 25 degrees Celsius; by subtracting 25 from the left column, you get the correlation between the temperature difference and the milli volt output.

Because the temperature scale moves in steps of 5 near 25 degrees and steps of 10 farther away, it is difficult to

index in an array. Therefore, it is beneficial to linearly interpolate between the temperature values so that the entire array is in steps of 5 degrees.

The thermopile voltage is amplified and then fed to the ADC. Therefore, you can construct a table that maps ADC voltages directly to a temperature difference.

## Read ADC Values

This function captures and accumulates 32 thermopile and thermistor values into variables tp\_avg and tr\_avg respectively. It then calculates the average of those values and stores the average in variables called tp and tr. Correlated doubling and IIR filtering is performed in this part of code.

## Process ADC Values for Temperature

The temperature is calculated from the thermistor resistance  $R_{th}$  and thermopile voltage  $V_{tp}$  values using the following algorithm:

- Check for overflow and underflow; if condition exists, exit with an error.
- Find the closest value in the appropriate table for the ADC value.
- Perform linear interpolation between the closest two values.
  - For the thermopile, the interpolation formula is as follows:

$$T_{tp} = -45 + 5i + 5 * \left( \frac{V_{tp} - U_{tp} Cal[i]}{U_{tp} Cal[i+1] - U_{tp} Cal[i]} \right)$$

- For the thermistor, the interpolation formula is follows:

$$T_a = -20 + 5i + 5 * \left( \frac{R_{th} - U_{th} Cal[i]}{U_{th} Cal[i+1] - U_{th} Cal[i]} \right)$$

Where

$U_{th}$  and  $U_{tp}$  are lookup table entries for thermistor and thermocouple respectively.

$i$  is the index of lookup table, or temperature

Ambient temperature can also be calculated from Stein Hart's equation:

$$T_c = \frac{1}{A + B \cdot \ln(R) + C \cdot \ln(R)^3} - 273.15$$

Where:

**A**, **B**, and **C** are empirical constants that are determined from thermistor characteristics

**R** is the thermistor's resistance in ohms.

**T<sub>c</sub>** is the temperature in Celsius.


To increase accuracy, temperature is calculated from ADC values using the polynomial provided by the sensor

manufacturer or from a bigger lookup table, which has much closer values of temperature.

Ambient temperature compensation is performed using Equation 10

$$\text{Equation 10} \quad T_{obj} = T_{tp} + T_a$$

Figure 7. PSoC Internal Routing Diagram

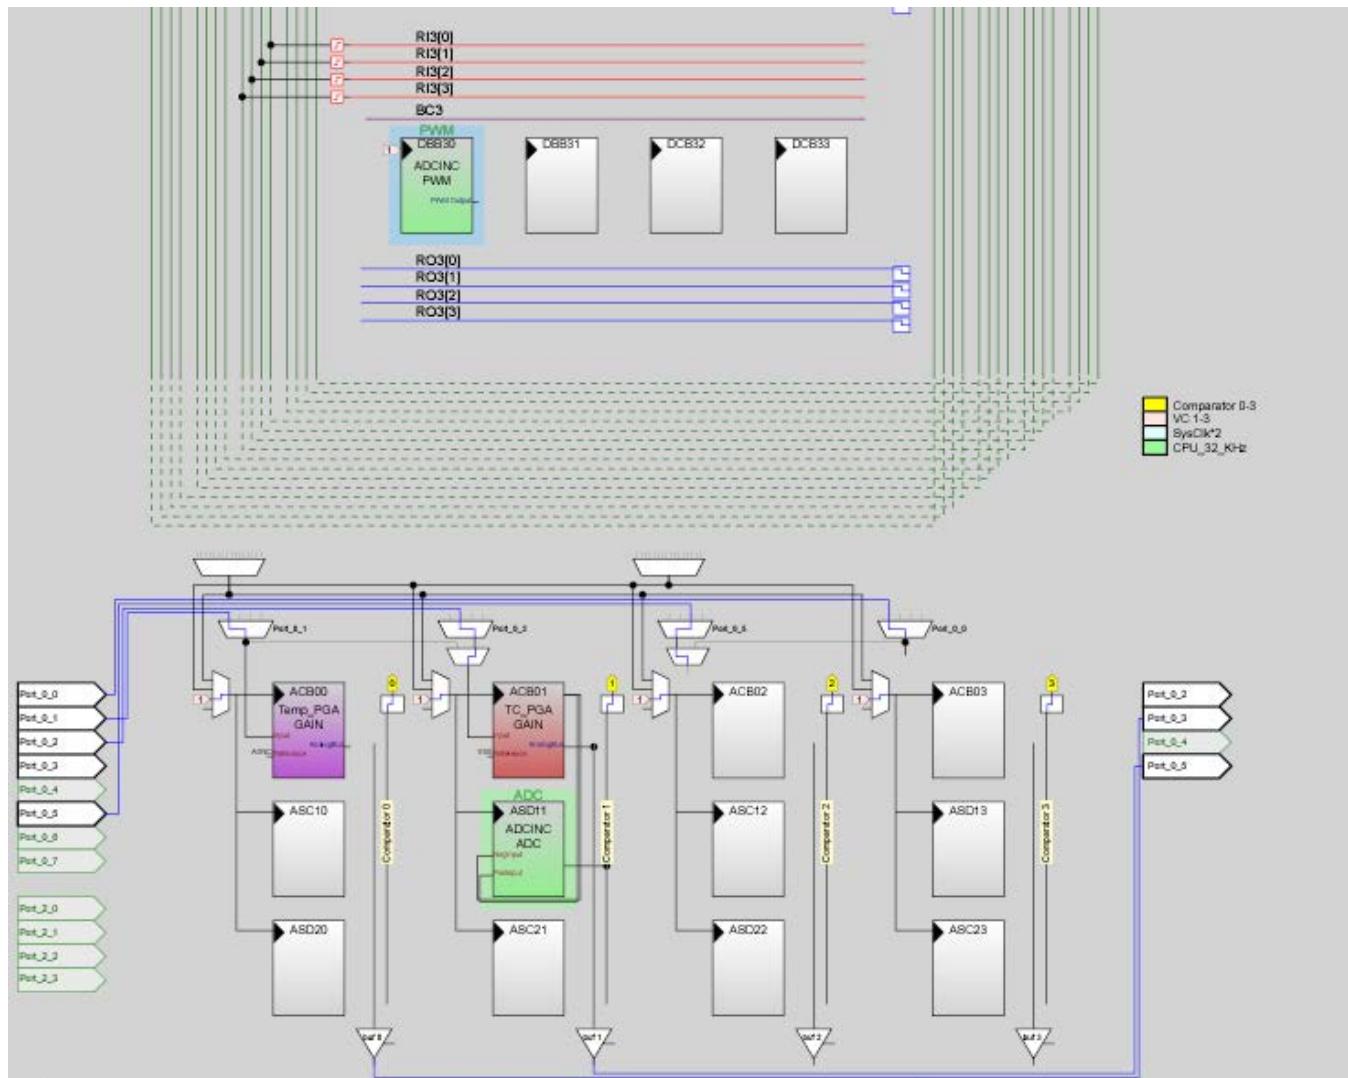

## Schematic

Figure 8 shows the schematic of infrared and Table 3 provides details of each net.

Figure 8. Schematic

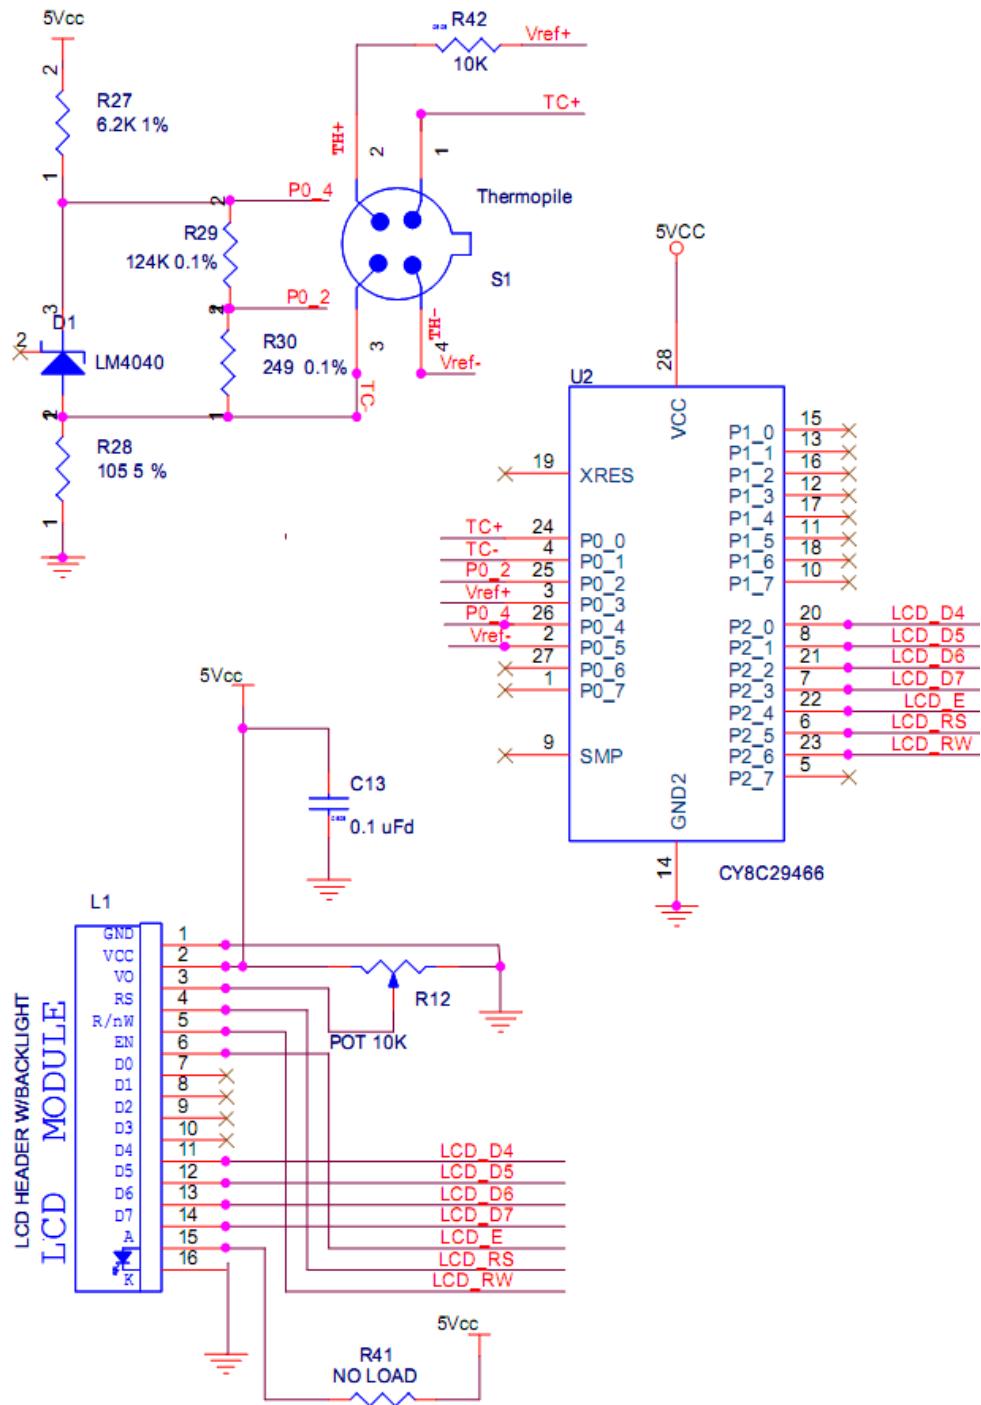


Table 3. Net Details

Net Name	Details
TH+ and TH-	Thermistor output of thermopile sensor
TC+ and TC-	Thermocouple output of thermopile sensor
AGND	Analog ground
LCD_xx	LCD data and control lines
Vref- and Vref+	Reference voltages from PSoC

## Accuracy of Object Temperature


The accuracy of object temperature depends on the following parameters. These parameters help to increase accuracy from 98 to 99 percent:

- Field of view angle (FOV) of IR radiation from object to sensor
- Type of casing and optics used in sensor
- Distance between sensor and object
- Calibration of the device

### Field of View Angle

FOV angle is the angular measure of the cone opening from which the sensor receives radiation as Figure 9 shows.

Figure 9. FOV Angle

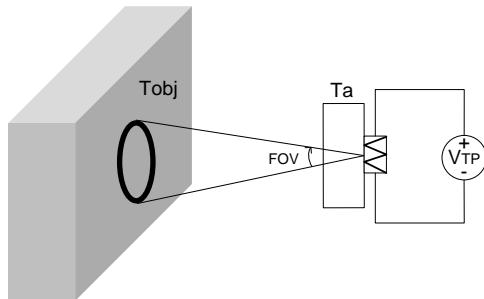


$V_{tp}$  varies with  $\sin^2(\text{FOV})$  and accuracy can be increased by keeping FOV nearer to 90 degrees.

### Casing and Optics in the Sensor

The type of casing used around the sensor affects its accuracy. Therefore, take special care when enclosing the sensor. More details of the case designing can be got from the sensor manufacturer. Figure 10 shows the casing built for Perkin Elmer TPS23B sensor. Sensor manufacturers can be contacted for more details about the design of casing.

Figure 10. Casing

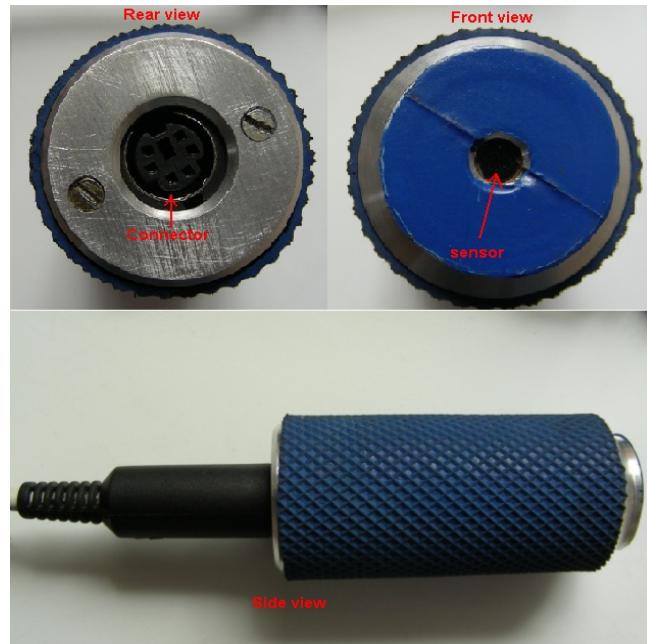

### Distance between Sensor and Object

The distance between the sensor and object produces a variation in readings. Therefore, the typical distance provided by the sensor manufacturer should be maintained. For sensor TPS23B, the distance is 2 to 3 cm. Proximity sense in PSoC can be used to maintain correct distance between sensor and object (human body) thereby reducing the error due to incorrect positioning.

## Calibration

Follow these steps for calibration:

1. Measure the offset of your device: The thermopile sensor is exposed to a complete thermal equilibrium in a closed environment. In front of the window, the same temperature is presented as the equilibrium temperature. Now the sensor gives 0 V, which is used to calibrate the offset of the electronics. Alternatively, a precise voltmeter is used for the thermopile output to measure how good the thermal equilibrium is.
2. The voltage  $V_{T_{Obj}}(\text{exp})$  is used to scale the sensors output in future and get a calibration constant  $k$ . From the table or from the polynomial, you get a voltage of a typical sensor  $V_{T_{Obj}}(\text{theor})$  by calculating:

$$V_{T_{Obj}}(\text{theor}) := V_{T_{Obj}}(\text{Radiation\_source}) - V_{T_{Obj}}(\text{Sensor})$$


Calibration constant  $k$  is calculated as

$$K = \frac{V_{T_{Obj}}(\text{theor})}{V_{T_{Obj}}(\text{Sensor})}$$

3. During measurements, all thermopile voltages must first be multiplied with  $k$  before further processing with polynomials of lookup-tables.

The look up table in the attached project is calibrated for the hardware setup including casing sensor etc.

Figure 11. IR Thermometer

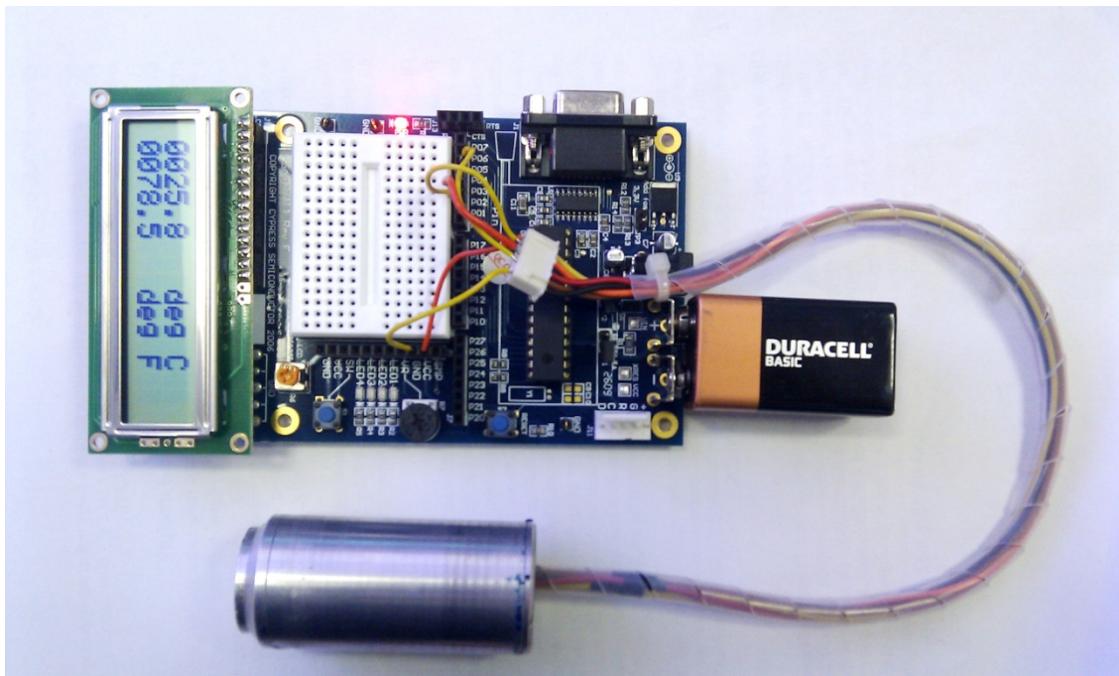

## Summary

This application note explains how to build an infrared thermometer with zero external active analog components. The project attached with this application note does not include any calibration routine.

## Related Application Notes

[AN2017](#) -- PSoC® 1 Temperature Measurement with Thermistor

[AN2226](#)-- PSoC® 1 -- Using Correlated Double Sampling to Reduce Offset, Drift, and Low Frequency Noise

[AN2099](#)-- PSoC® 1, PSoC 3, and PSoC 5LP— Single-Pole Infinite Impulse Response (IIR) Filters

## About the Author

Name: Sanjeev Kumar. K

Title: Applications Engineer

Background: Sanjeev has a bachelor's degree in Electronics and Communication from the College of Engineering, Guindy, Chennai. He currently works on PSoC based applications at Cypress.

Contact: [kuk@cypress.com](mailto:kuk@cypress.com)

## Document History

Document Title: Infrared Thermometer using PSoC® - AN58829

Document Number: 001-58829

Revision	ECN	Orig. of Change	Submission Date	Description of Change
**	2855922	KUK	1/18/10	New application note
*A	3126363	KUK	01/03/2011	Software version changed from PSoC designer 5.0 to 5.1 Device name in abstract updated from PSoC® to PSoC® 1 AN Changed from CapSense category to PSoC1 category Updated details on casing Updated project to PSoC designer 5.1
*B	3941788	KUK	03/22/2013	Software Version as "PSoC® Designer™ 5.3". Updated Abstract. Updated Infrared Thermometer Principle (Updated Figure 2 and Figure 3). Removed the Note "Medical demo daughter card is build for internal cypress demo and the same is not sold in cypress web." below Figure 11. Updated Summary. Updated to new template. Updated project to PSoC designer 5.3. Updated code to match latest CY coding standards.
*C	4729551	ASRI	04/17/2015	Updated Software Version "PSoC® Designer™ 5.4" in page 1. Updated attached associated project with PSoC designer 5.4. Updated to new template. Completing Sunset Review.

## Worldwide Sales and Design Support

Cypress maintains a worldwide network of offices, solution centers, manufacturer's representatives, and distributors. To find the office closest to you, visit us at [Cypress Locations](#).

## Products

Automotive	<a href="http://cypress.com/go/automotive">cypress.com/go/automotive</a>
Clocks & Buffers	<a href="http://cypress.com/go/clocks">cypress.com/go/clocks</a>
Interface	<a href="http://cypress.com/go/interface">cypress.com/go/interface</a>
Lighting & Power Control	<a href="http://cypress.com/go/powerpsoc">cypress.com/go/powerpsoc</a> <a href="http://cypress.com/go/plc">cypress.com/go/plc</a>
Memory	<a href="http://cypress.com/go/memory">cypress.com/go/memory</a>
PSoC	<a href="http://cypress.com/go/psoc">cypress.com/go/psoc</a>
Touch Sensing	<a href="http://cypress.com/go/touch">cypress.com/go/touch</a>
USB Controllers	<a href="http://cypress.com/go/usb">cypress.com/go/usb</a>
Wireless/RF	<a href="http://cypress.com/go/wireless">cypress.com/go/wireless</a>

## PSoC® Solutions

[psoc.cypress.com/solutions](http://psoc.cypress.com/solutions)  
[PSoC 1](#) | [PSoC 3](#) | [PSoC 4](#) | [PSoC 5LP](#)

## Cypress Developer Community

[Community](#) | [Forums](#) | [Blogs](#) | [Video](#) | [Training](#)

## Technical Support

[cypress.com/go/support](http://cypress.com/go/support)

PSoC is a registered trademark of Cypress Semiconductor Corp. "Programmable System-on-Chip" and PSoC Designer are trademarks of Cypress Semiconductor Corp. All other trademarks or registered trademarks referenced herein are the property of their respective owners.



© Cypress Semiconductor Corporation, 2010-2015. The information contained herein is subject to change without notice. Cypress Semiconductor Corporation assumes no responsibility for the use of any circuitry other than circuitry embodied in a Cypress product. Nor does it convey or imply any license under patent or other rights. Cypress products are not warranted nor intended to be used for medical, life support, life saving, critical control or safety applications, unless pursuant to an express written agreement with Cypress. Furthermore, Cypress does not authorize its products for use as critical components in life-support systems where a malfunction or failure may reasonably be expected to result in significant injury to the user. The inclusion of Cypress products in life-support systems application implies that the manufacturer assumes all risk of such use and in doing so indemnifies Cypress against all charges.

This Source Code (software and/or firmware) is owned by Cypress Semiconductor Corporation (Cypress) and is protected by and subject to worldwide patent protection (United States and foreign), United States copyright laws and international treaty provisions. Cypress hereby grants to licensee a personal, non-exclusive, non-transferable license to copy, use, modify, create derivative works of, and compile the Cypress Source Code and derivative works for the sole purpose of creating custom software and/or firmware in support of licensee product to be used only in conjunction with a Cypress integrated circuit as specified in the applicable agreement. Any reproduction, modification, translation, compilation, or representation of this Source Code except as specified above is prohibited without the express written permission of Cypress.

Disclaimer: CYPRESS MAKES NO WARRANTY OF ANY KIND, EXPRESS OR IMPLIED, WITH REGARD TO THIS MATERIAL, INCLUDING, BUT NOT LIMITED TO, THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. Cypress reserves the right to make changes without further notice to the materials described herein. Cypress does not assume any liability arising out of the application or use of any product or circuit described herein. Cypress does not authorize its products for use as critical components in life-support systems where a malfunction or failure may reasonably be expected to result in significant injury to the user. The inclusion of Cypress' product in a life-support systems application implies that the manufacturer assumes all risk of such use and in doing so indemnifies Cypress against all charges.

Use may be limited by and subject to the applicable Cypress software license agreement.